

Design and implementation of a reflection pulse oximeter in tele-monitoring system

Xinsheng Lv*, Jinling Zhang, Xiongzi Zhu, Jun Wang, Yubo Chen
School of electronic engineering
Beijing University of Posts and Telecommunications
Beijing, China
*lwlxsh@163.com

Abstract—Pulse oxygen saturation is an important physiological parameter for monitoring oxygen content and respiratory function. It is very inconvenient that the pulse oximeter in the hospital use transmission probe and the data measurement have to be done in close range. Therefore, this paper designed a reflection pulse oximeter in tele-monitoring system. Firstly, a reflection oximeter which is based on reflection sensor DCM03 and microcontroller MSP430 is designed. Subsequently, Zigbee wireless module is integrated on the circuit board to realize remote measurement. Finally, the second derivative of photoplethysmography waveform derived from photoplethysmography signal is analyzed. Some experiments are conducted in the end and the method proposed maybe help confirming the relationship between SDPPG (second derivative of photoplethysmography) and human tired or diseases.

Keywords—Reflection; Zigbee; tele-monitoring system; SDPPG; heart rate

I. INTRODUCTION

Non-invasive pulse oximetry is a safe, reliable, real time and continuous measurement method and has been widely used in clinical care. Nowadays transmittance oximetry has been fully developed and there're many mature products which are widely used in hospitals [1]. However, a transmittance pulse oximeter practical only in case the patient is in hospital or lying steadily. Besides, transmittance measurements sometimes cause uncomfortable because its sensor presses a finger or ear lobe. The reflection pulse oximeter can increase the flexibility and avoid the problems above, whereas the research of reflectance oximeter is still immaturity [2]. At present, the PPG monitoring system used in the hospital receive the PPG signal through wire and the data can't be observed by the people who are not in this region, which is extremely inconvenience. However the system designed by us solves the problems above. In addition, the reflection oximeter we design is more convenience than the transmittance one because we need to contact to the sensor only rather than put the finger or ear lobe in the transmission oxygen probe

In this paper, we design a reflection pulse oximeter using sensor DCM03 made by APMKorea and microcontroller MSP430FG43x made by TI. In order to meet the needs of modern community healthcare, we design a reflection pulse oxygen saturation tele-monitoring system using Zigbee wireless module and GPRS network system [3] [4]. We also accomplish some experiments used the reflection oximeter we

designed to prove whether is there relationship between SDPPG and human tired or diseases.

The paper is organized as follows. The system architecture is introduced in Section II. The design of the reflection oximeter is described in Section III. Simulation results and data analyses are presented in Section IV. Finally, the conclusions are summarized in Section V.

II. SYSTEM ARCHITECTURE

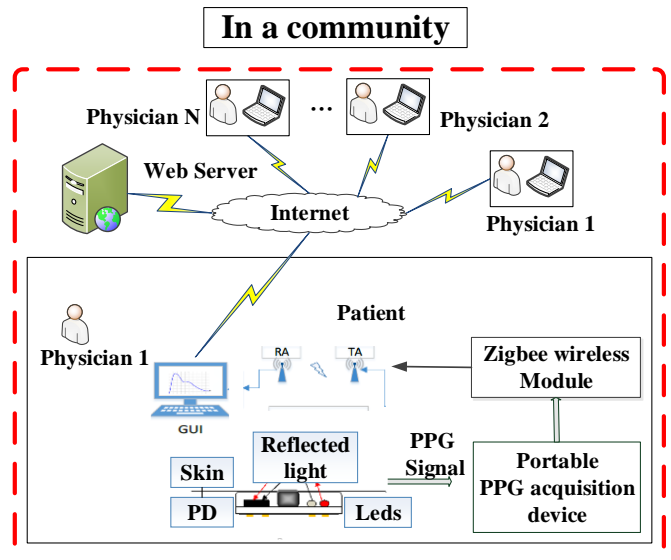


Fig. 1 Diagram of the system architecture

The diagram of the architecture of the reflection pulse oxygen saturation tele-monitoring system is showed in Fig.1. In this system, the PPG (photoplethysmography) signals are obtained by reflection sensor and processed by the portable PPG acquisition device. After the PPG signals are acquired by the device, if people and physicians are in a community, the Zigbee wireless module integrated on the portable device will transmit the PPG signal and the value of the SpO2 and the PR which are processed and calculated by the device to the display interface on the computer in real time. At the same time, the display interface upload the data to the web server, so that the physicians out of the community can observe the data. The physicians and the people themselves can observe

through the arteries, so the SpO_2 and the HR (heart rate) can be calculated in the microcontroller now.

All of the works showed above can be done only needing a microcontroller MSP430FG43x apart from four transistors that used to control the light intensity of the LEDs and a few passive components. OAs and ADCs integrated in the MSP430 is one important reason why we choose MSP430 as the main microcontroller. Another important reason is that it provides a very low power consumption characteristic, while this is important for the portable acquisition device.

There is one important problem to be solved now. It is getting the values of a and b in formula (2) to calculate the values of the SpO_2 . To get the values, a tool named oxygen saturation simulator is needed. It will tell us the relationship of the SpO_2 and R. By doing a few experiments, a curve about SpO_2 and R is available. We can calculate the value of a and b by this curve, this process is well known as the experimental calibration.



Fig. 4 Picture of the portable reflection oximeter

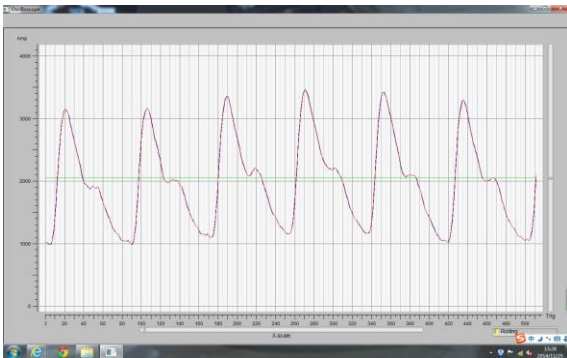


Fig. 5 The PPG signal on the display interface

The HR is measured by calculating the cycle of pulse wave signal. Finally, the MSP430 is used to calculate the SpO_2 and HR, and display the values of them on the OLED or transport them and the PPG waves to the PC via Zigbee wireless module continuously. Fig. 4 shows the picture of the portable reflection pulse oxygen saturation acquisition device. The number in the top of the OLED is the value of SpO_2 and the one in the bottom of the OLED is the value of HR or PR. The Zigbee wireless module was integrated on the circuit board in the box to transmit data. As is shown in the Fig. 5, the pulse waves on the display interface we get via the device we design is very smoothness. All of these improve that our design of the reflection pulse oxygen saturation acquisition device is

applicable.

IV. DATA ANALYSIS OF THE PPG WAVES

As we all know, the PPG is a noninvasive method to measure blood volume change. At the end of the paper, we prove that the SDPPG derived from the PPG can be used to monitor the arterial condition, while the data of the PPG signals were recorded from the portable reflection pulse oximeter we designed.

Five healthy volunteers take part in this analysis. The data of SDPPG were analyzed off-line using MATLAB. We extract the data of pulse waveforms through software, and handle the data using MATLAB. The PPG signal of volunteer A1 are shown in Fig. 6, while the FDPPG (first derivative of PPG) was shown in Fig. 7.

The SDPPG waveform for volunteer A1 is showed in Fig. 8. It consists of the initial positive wave (a wave), early negative wave (b wave), re-uploping wave (c wave), late downsloping wave (d wave), and diastolic positive wave (e wave) and the shift from the baseline to the peak of each wave is taken as the value for each wave. The SDPPG wave pattern is determined by the proportions of the b, c, d and e waves to the a wave [5].

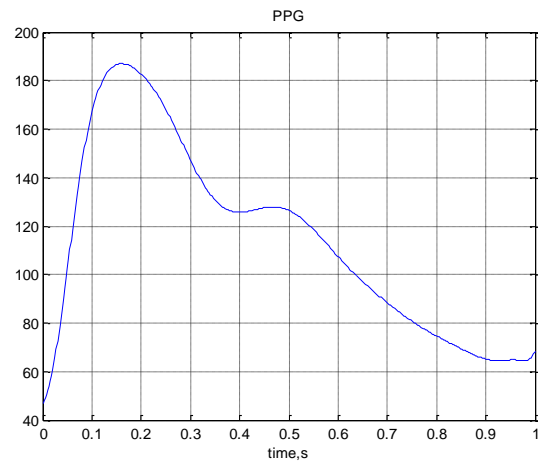


Fig. 6 PPG waveform of normalized finger for subject A1

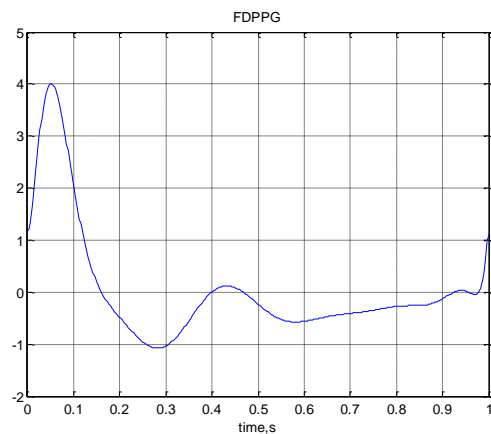


Fig. 7 First derivative signal of PPG

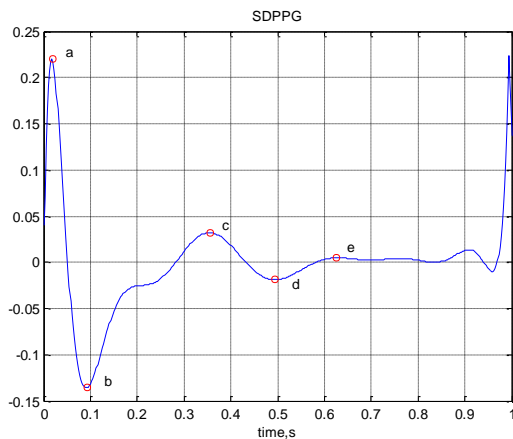


Fig. 8 SDPPG waveform for subject A1

TABLE I. Summary of data for study sample

Subject		SDPPG-AI	SDPPG-AI
No.	Age(years)	(volunteers')	(not real data)
A1	23	-0.79±0.03	-0.71±0.11
A2	24	-0.81±0.15	-0.72±0.13
A3	25	-0.84±0.18	-0.75±0.07
A4	25	-0.86±0.22	-0.78±0.20
A5	24	-0.73±0.16	-0.69±0.14

SDPPG aging index (SDPPG-AI) can be calculated by the equation (3).

$$SDPPG-AI = \frac{(b-c-d-e)}{a} \quad (3)$$

The values of a, b, c, d and e were got from the MATLAB. As shown in Fig. 8, the ordinate value of point a is the ordinate value of the first positive extreme point in one cycle, while the ordinate value of point b is the ordinate value of the first negative extreme point in the same circle. The rest c, d and e can be done in the same manner. Then we calculate the values of the SDPPG-AI and do some analysis. We estimate the human tired and some diseases may be related to the SDPPG-AI, and now we are conducting some experiments, but because the number of the samples is too small, we don't show the data analysis here. But we are sure of that we can employ the data obtained from the reflection oximeter we design to do some analysis about human tired and some diseases.

Fig. 9 shows the comparison of SDPPG-AI for healthy volunteers and a set of unreal data. The mean and standard deviation of SDPPG-AI are displayed in Table 1. The left part of table 1 was obtained by the device we designed, while the data of the right part were comparative data that we set. We just want to declare that we can analyze the relationship between SDPPG-AI obtained from the reflection oximeter we designed and tired or some diseases through the data comparison. We believe that the comparison about SDPPG-AI obtained from the reflection oximeter may be a useful method to evaluate the human tired and diseases in the future.

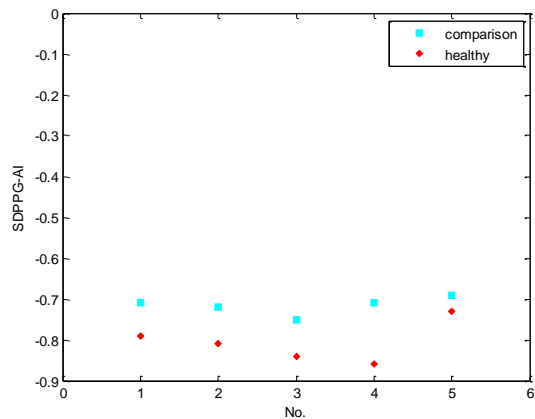


Fig. 9 SDPPG-AI for each volunteer

CONCLUSION

This paper describes the Design and implementation of a reflection pulse oximeter in tele-monitoring system. The reflection oximeter we design can obtain oxygen saturation and heart rate information continuously, non-invasively and real-time through a reflection sensor DCM03. The system is a tele-monitoring system using Zigbee wireless module and GPRS network. Therefore, it is suitable for real time and remote monitoring. In the end of the paper, we thought that there may be some relationship between SDPPG-AI and some diseases and human tired. But we have a lot of work to do to prove it. We believe that detecting the SDPPG waveform may be a useful method to monitor human health in the future.

ACKNOWLEDGMENT

Our researches are supported by a grant from the technological innovation fund project of scientific and technological enterprises in Jiangsu Province (No. SBC201310543). The authors would like to thank our colleagues in the laboratory for their technical assistance.

REFERENCES

- [1] Miia M, Antti K, Esko A, and YoungChung W. "Optimum Place for Measuring Pulse Oximeter Signal in Wireless Sensor-Belt or Wrist-Band," International Conference on Convergence Information Technology. Gyeongju. pp. 1856-1861, Nov 2007.
- [2] O. Abdallah, A. Bolz. "Signal Processing by Reflectance Pulse Oximetry for Monitoring the fractional Oxygen Saturation and the Detektion of Anemia," IFMBE Proceedings. pp. 1152-1155.
- [3] Jinling Zhang, Jun Wang, Xin-sheng Lv, and Yunpeng Han, "Design of Health Monitoring Platform Base on Medical Wisdom," Applied Mechanics and Materials (in Chinese). Vol. 644-650. pp. 1062-1065, Sep 2014.
- [4] Jinling Zhang, Jun Wang, Lei Shu, and Sheng Zhang, "Design of Data Management System for Remote ECG Monitoring," Applied Mechanics and Materials (in Chinese). pp. 993-996, Mar 2014.
- [5] Hyun Jae Baek, Jung Soo Kim, Yun Sung Kim, Haet Bit Lee and Kwang Suk Park, "Second derivative of photoplethysmography for estimating vascular aging," 6th Int'l Special Topic Conference on ITAB. Tokyo. pp. 70-73, Nov 2007.
- [6] Guowei Di, Xiaoying Tang, and Weifeng Liu, "A Reflectance Pulse Oximeter Design Using the MSP430F149," Complex Medical Engineering (in Chinese). Beijing. pp. 1081-1084, May 2007.